
DRILLING PROTOCOL STRAUMANN BLC™/TLC™

straumann


Drilling Protocol Videos

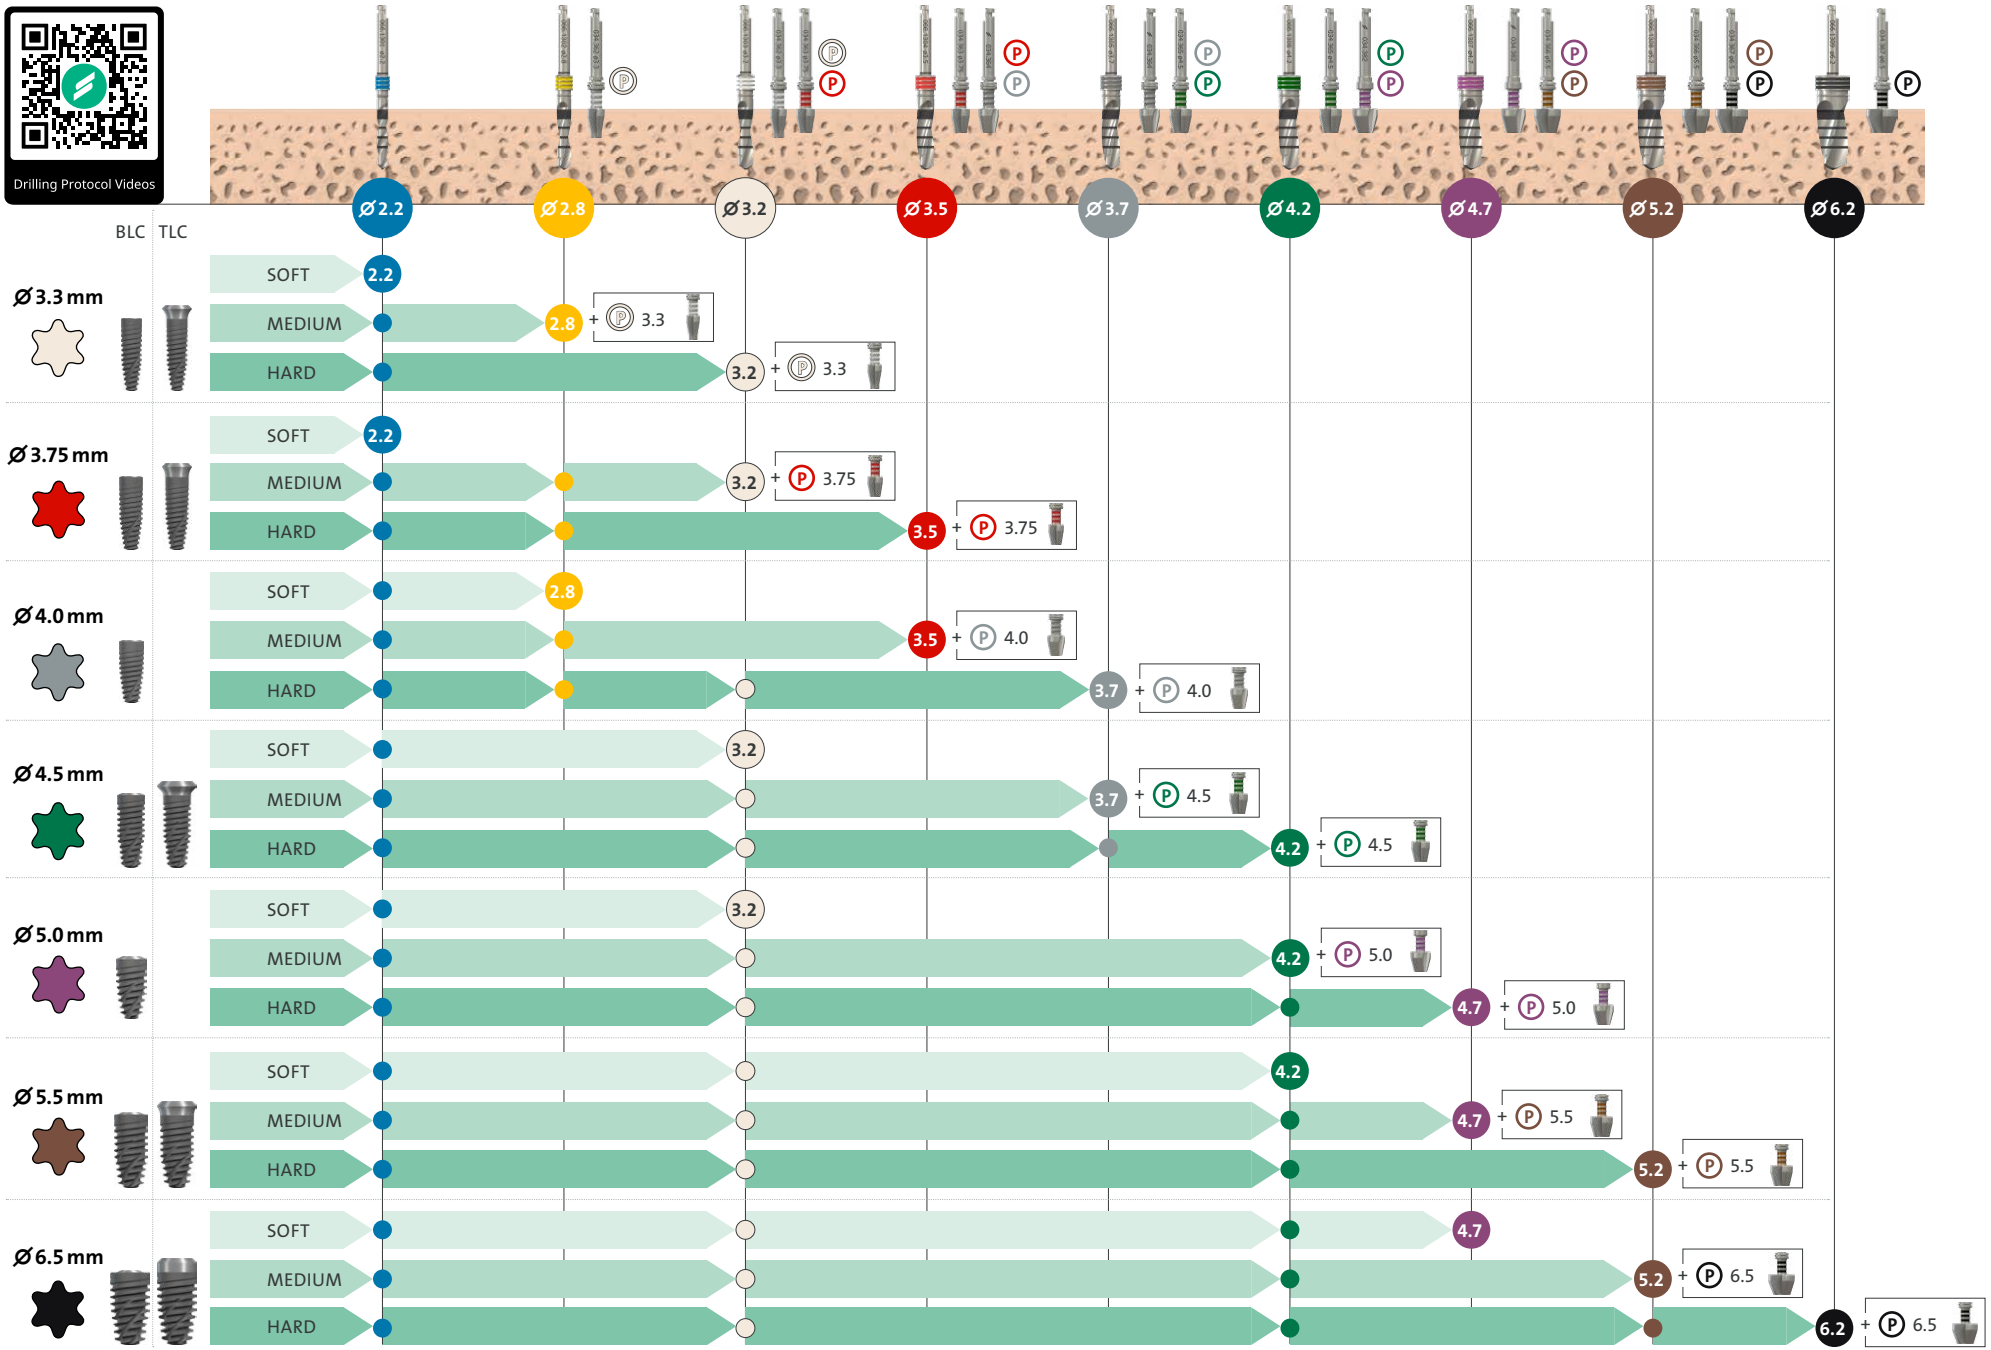

DRILLING PROTOCOL STRAUMANN BLX™/TLX™

straumann

Drilling Protocol Videos

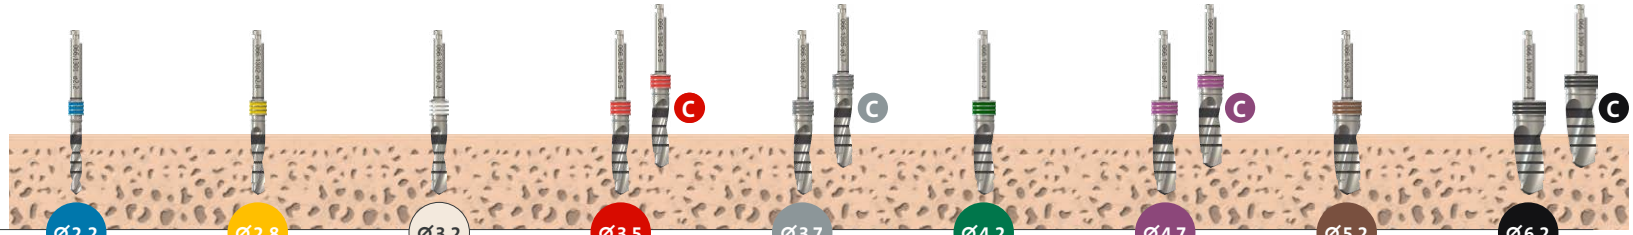

	BLX	TLX		Ø2.2	Ø2.8	Ø3.2	Ø3.5	Ø3.7	Ø4.2	Ø4.7	Ø5.2	Ø6.2
Ø3.5 mm	●		SOFT	2.2								
			MEDIUM	●	2.8		C					
			HARD	●		3.2	C					
Ø3.75 mm	●	●	SOFT	●	2.8							
			MEDIUM	●	●	3.2		C				
			HARD	●	●		3.5	C				
Ø4.0 mm	●	●	SOFT	●	2.8							
			MEDIUM	●	●		3.5	C				
			HARD	●	●	○		3.7				
Ø4.5 mm	●	●	SOFT	C*	2.8							
			MEDIUM	●		○		3.7				
			HARD	●		○		●	4.2			
Ø5.0 mm	●	●	SOFT	●		3.2						
			MEDIUM	●		○			4.2	C		
			HARD	●		○			●	4.7		
Ø5.5 mm	●	●	SOFT	●		3.2						
			MEDIUM	●		○			●	4.7		
			HARD	●		○			●	●	5.2	
Ø6.5 mm	●	●	SOFT	●		○	3.5					
			MEDIUM	●		○			●		5.2	C
			HARD	●		○			●		●	6.2

(C) Cortical Bone
→ Implant 6 mm - 8 mm: Drill depth 4 mm
→ Implant 10 mm - 18 mm: Drill depth 6 mm

* The implant bed preparation for 4 mm implants ends here: Implant 4 mm

International Headquarters
Institut Straumann AG
Peter Merian-Weg 12
CH-4002 Basel, Switzerland
Phone +41 (0)61 965 11 11
Fax +41 (0)61 965 11 01
www.straumann.com

© Institut Straumann AG, 2026. All rights reserved. Straumann® and/or other trademarks and logos from Straumann® mentioned herein are the trademarks or registered trademarks of Straumann Holding AG and/or its affiliates.

041.790/en/F/05 04/26
707786/en/F/05 04/26