straumann в Україні

Technical Informa



Straumann®

iExcel (BLX, BLC, TLX, TLC)

Basic Information

WHITE


straumann

Імплантат BLX. Конструкція та специфікація


	Straumann® BLX Implant						
	Ø 3.5 mm	Ø 3.75 mm	Ø 4.0 mm	Ø 4.5 mm	Ø 5.0 mm	Ø 5.5 mm	Ø 6.5 mm
[A] Maximum outer diameter	Ø 3.5 mm	Ø 3.75 mm	Ø 4.0 mm	Ø 4.5 mm	Ø 5.0 mm	Ø 5.5 mm	Ø 6.5 mm
[B] Neck diameter	Ø 3.4 mm	Ø 3.5 mm			Ø 4.5 mm		
[C] Platform diameter	Ø 2.9 mm						
[D] Connection diameter	Ø 2.7 mm						
[E] 22.5° bevel height	0.1 mm	0.12 mm			0.33 mm		
[F] Apical diameter, body	Ø 1.9 mm				Ø 2.2 mm		
[G] Apical diameter, threads	Ø 2.75 mm	Ø 2.9 mm		Ø 3.6 mm	Ø 3.5 mm	Ø 4.0 mm	Ø 5.2 mm
Number of apical cutting edges	2				4		
[L] Implant lengths: 6 mm, 8 mm							
[H] Neck height	1.0 mm						
[M] Micro threads height	0.5 mm						
[P] Thread pitch*	1.7 mm		1.8 mm	2.0 mm	1.9 mm	2.1 mm	2.3 mm
[T] Thread spacing	0.85 mm		0.9 mm	1.0 mm	0.95 mm	1.05 mm	1.15 mm
[L] Implant lengths: 10 mm, 12 mm, 14 mm							
[H] Neck height	1.7 mm						
[M] Micro threads height	0.85 mm						
[P] Thread pitch*	2.1 mm	2.2 mm	2.25 mm	2.5 mm	2.3 mm	2.5 mm	2.7 mm
[T] Thread spacing	1.05 mm	1.1 mm	1.125 mm	1.25 mm	1.15 mm	1.25 mm	1.35 mm
[L] Implant lengths: 16 mm, 18 mm							
[H] Neck height	2.0 mm						
[M] Micro threads height	1.0 mm						
[P] Thread pitch*	2.5 mm	2.6 mm	2.7 mm	2.8 mm	2.7 mm	2.8 mm	3.1 mm
[T] Thread spacing	1.25 mm	1.3 mm	1.35 mm	1.4 mm	1.35 mm	1.4 mm	1.55 mm

* Implant advances by this amount with every rotation.

Straumann®
BLX Implant
Ø 4.5 mm

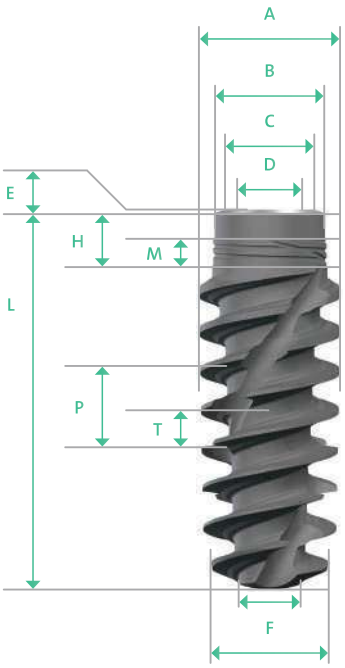


Імплантат BLC. Конструкція та специфікація

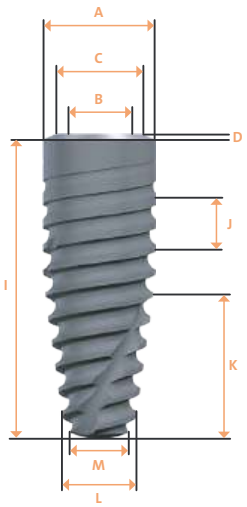

	Straumann BLC™ Implants						
	BLC Ø3.3mm RB	BLC Ø3.75 mm RB	BLC Ø4.0mm RB	BLC Ø4.5mm WB	BLC Ø5.0mm WB	BLC Ø5.5mm WB	BLC Ø6.5mm WB
(A) Maximum implant body outer diameter	3.3 mm	3.75 mm	4.0 mm	4.5 mm	5.0 mm	5.5 mm	6.5 mm
(B) Connection diameter	2.7 mm						
(C) Platform diameter	2.9 mm						
(D) 22.5° bevel height	0.1 mm	0.18 mm	0.23 mm	0.33 mm			
(I) Endosteal lengths	8-18 mm	6-18 mm				6-16 mm	
(J) Thread pitch*/flank lead/ depth	1.6 mm/20°/0.35 mm		1.6 mm/ 20°/ 0.35 mm	1.8 mm/20°/0.45 mm	2.1 mm/ 20°/ 1.05	2.1 mm/ 20°/ 0.5 mm	2.3 mm/ 20°/ 0.75 mm
Number of chip flutes	2			2 for L 6 mm/ 4 for L 8-18 mm		4	
Implant lengths: 6 to 8 mm							
(K) Tapered part/taper	2.6 mm/14°			2.7 mm/14°	2.6 mm/14°		
(L) Apical diameter threads	2.22 mm	2.63 mm	2.88 mm	3.5 mm	4.1 mm	4.63 mm	5.71 mm
(M) Apical diameter core	1.52 mm	1.81 mm	2.18 mm	2.36 mm	2.75 mm	3.18 mm	3.67 mm
Implant lengths: 10 to 18 mm							
(K) Tapered part/taper	5 mm/8°	5.2 mm/8°	4.8 mm/8°	5.5 mm/8°			6.5 mm/8°
(L) Apical diameter threads	2.05 mm	2.37 mm	2.76 mm	3.10 mm	3.62 mm	4.14 mm	4.87 mm
(M) Apical diameter core	1.35 mm	1.61 mm	2.10 mm		1.79 mm	2.21 mm	2.76 mm


* Implant advances by this amount with every rotation.

Гібридне з’єднання TorcFit ™

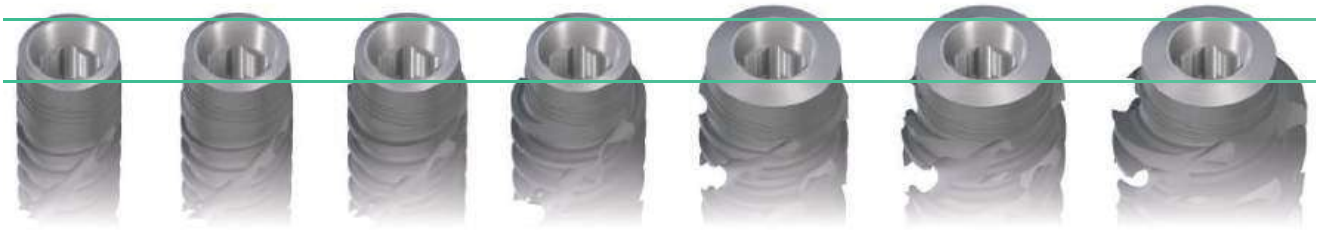

Ø 3.5 mm | Ø 3.75 mm | Ø 4.0 mm | Ø 4.5 mm | Ø 5.0 mm | Ø 5.5 mm | Ø 6.5 mm

· зіркоподібне з’єднання · 7° конус Morse · зовнішнє багатофункціональне плече · тактильне відчуття правильного розміщення

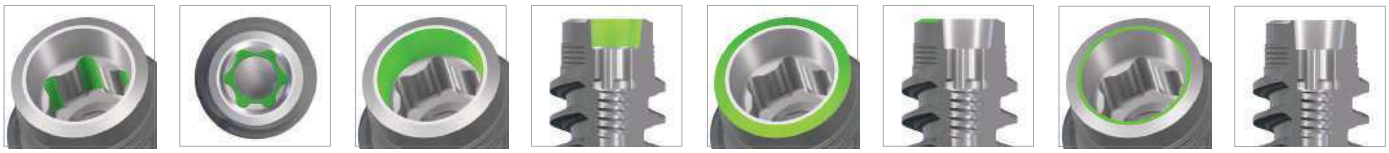


Модульна касета Straumann® iExcel

С-модуль, Допоміжний набір
041.783



В Модуль, Лоток TorcFit™ BLC, TLC, BLX, TLX
041.787

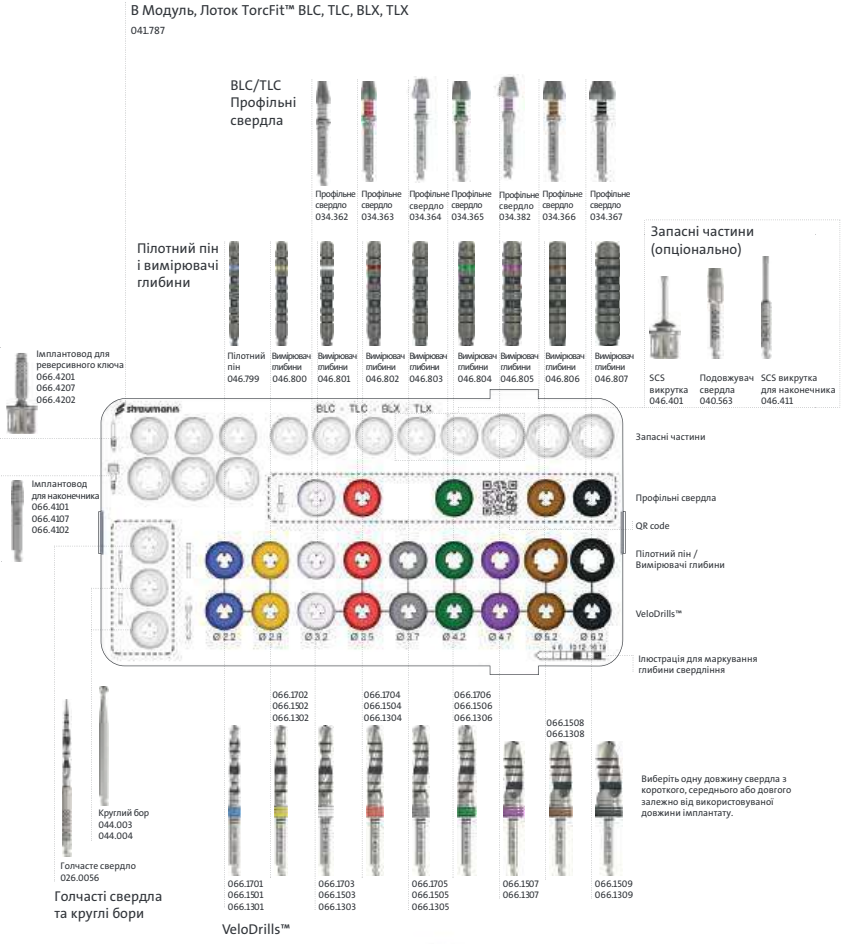



Модульна касета Straumann® використовується для стерилізації та безпечного зберігання хірургічних та допоміжних інструментів.

Straumann®
BLX/BLC Implant System
System Overview

BLX/BLC SURGERY

	Ø 3.3 mm		Ø 3.5 mm		Ø 3.75 mm			
	BLC		BLX		BLC		BLX	
	RB (Regular Base)		RB (Regular Base)		RB (Regular Base)		RB (Regular Base)	
								
	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®
Implants								
6 mm	–	–	–	–	035.9206S	035.8206S	061.4306	061.4506
8 mm	035.9008S	035.8008S	061.3308	061.3508	035.9208S	035.8208S	061.4308	061.4508
10 mm	035.9010S	035.8010S	061.3310	061.3510	035.9210S	035.8210S	061.4310	061.4510
12 mm	035.9012S	035.8012S	061.3312	061.3512	035.9212S	035.8212S	061.4312	061.4512
14 mm	035.9014S	035.8014S	061.3314	061.3514	035.9214S	035.8214S	061.4314	061.4514
16 mm	035.9016S	035.8016S	061.3316	061.3516	035.9216S	035.8216S	061.4316	061.4516
18 mm	035.9018S	035.8018S	061.3318	061.3518	035.9218S	035.8218S	061.4318	061.4518

Implant Drivers



Surgical Handle
066.4000



Short, L 21 mm
066.4101

VeloDrill™
Alignment Pins
Depth Gauges
Profile Drills

Drill No. 1 (Pilot Drill)



Ø 2.2 mm	
Short, L 34 mm	066.1301
Medium, L 38 mm	066.1501
Long, L 42 mm	066.1701



Alignment Pin	046.799

Drill No. 2



Ø 2.8 mm	
Short, L 34 mm	066.1302
Medium, L 38 mm	066.1502
Long, L 42 mm	066.1702



Depth Gauge	046.800

RB (Regular Base)

Closure Cap
H 0.4 mm / 2 mm



064.4100S



064.4101S

Healing Abutment



AH = abutment height
GH = gingiva height
Ø = diameter

Healing Abutments for Crown, AH 2 mm

	Diameter (Ø)			
GH	Ø 4.0 mm	Ø 5.0 mm	Ø 6.5 mm	Ø 7.5 mm
				
1.5 mm	064.4202S	064.4212S	064.4222S	–
2.5 mm	064.4204S	064.4214S	064.4224S	064.4234S*
3.5 mm	064.4206S	064.4216S	064.4226S	064.4236S*

Auxiliary Instruments

Torque Control Device		066.1100
Ratchet		046.119
Holding Key		046.064
Implant depth gauge		066.2000

Ø 4.0 mm

BLC
RB (Regular Base)



BLX
RB (Regular Base)



Ø 4.5 mm

BLC
WB (Wide Base)



BLX
RB (Regular Base)



	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®
6 mm	035.9306S	035.8306S	061.5306	061.5506	035.9406S	035.8406S	061.6306	061.6506
8 mm	035.9308S	035.8308S	061.5308	061.5508	035.9408S	035.8408S	061.6308	061.6508
10 mm	035.9310S	035.8310S	061.5310	061.5510	035.9410S	035.8410S	061.6310	061.6510
12 mm	035.9312S	035.8312S	061.5312	061.5512	035.9412S	035.8412S	061.6312	061.6512
14 mm	035.9314S	035.8314S	061.5314	061.5514	035.9414S	035.8414S	061.6314	061.6514
16 mm	035.9316S	035.8316S	061.5316	061.5516	035.9416S	035.8416S	061.6316	061.6516
18 mm	035.9318S	035.8318S	061.5318	061.5518	035.9418S	035.8418S	061.6318	061.6518



Medium, L 26 mm
066.4107



Long, L 31 mm
066.4102



Extra Long, L 36 mm
066.4108



Short, L 21 mm
066.4201

Drill No. 3

	Ø 3.2 mm	
	Short, L 34 mm	066.1303
	Medium, L 38 mm	066.1503
	Long, L 42 mm	066.1703
	Depth Gauge	046.801
	Profile Drills, Ø 3.3mm	034.362

Drill No. 4

	Ø 3.5 mm	
	Short, L 34 mm	066.1304
	Medium, L 38 mm	066.1504
	Long, L 42 mm	066.1704
	Depth Gauge	046.802
	Profile Drills, Ø 3.75 mm	034.363

Drill No. 5

	Ø 3.7 mm	
	Short, L 34 mm	066.1305
	Medium, L 38 mm	066.1505
	Long, L 42 mm	066.1705
	Depth Gauge	046.803
	Profile Drills, Ø 4.0 mm	034.364

RB (Regular Base)



064.4100S



064.4101S

Healing Abutments for Crown, AH 4 mm

GH	Diameter (Ø) Ø 4.0 mm	Ø 5.0 mm	Ø 6.5 mm	Ø 7.5 mm
				
1.5 mm	064.4203S	064.4213S	064.4223S	–
2.5 mm	064.4205S	064.4215S	064.4225S	064.4235S*
3.5 mm	064.4207S	064.4217S	064.4227S	064.4237S*

Healing Abutment for Bridge, AH 2 mm

GH	Diameter (⊠) Ø 5.0 mm
1.5 mm	 064.4232S

Healing Abutment for Bridge, AH 4 mm

GH	Diameter (⊠) Ø 5.0 mm
1.5 mm	 064.4233S

BL Bone Profiler Kit

BL Bone Profiler 1		026.0022
BL Bone Profiler 2		026.0023
BL Bone Profiler 3		026.0024
Guiding Pin for BLX/BLC Implants		066.0025S

Anatomic Healing Abutments XC (AHA)

Shape	S 	S1 	M 	XL 		
Ø and Platform	Ø 3.8 mm RB/WB	Ø 3.8 mm RB/WB	Ø 3.8 mm RB/WB	Ø 4.5 mm RB/WB	Ø 5.5 mm WB	Ø 6.5 mm WB
GH 1.5 mm	064.4432S	064.4514S	064.4452S	064.4482S	064.8482S	064.4522S
GM 2.5 mm	064.4433S	064.4515S	064.4453S	064.4483S	064.4510S	064.4523S

Straumann®
BLX/BLC Implant System
System Overview

BLX/BLC SURGERY

Ø 5.0 mm

BLC

WB (Wide Base)



BLX

WB (Wide Base)



Implants

	BLC Roxolid® SLActive®	BLC Roxolid® SLA®	BLX Roxolid® SLActive®	BLX Roxolid® SLA®
6 mm	035.9506S	035.8506S	061.7306	061.7506
8 mm	035.9508S	035.8508S	061.7308	061.7508
10 mm	035.9510S	035.8510S	061.7310	061.7510
12 mm	035.9512S	035.8512S	061.7312	061.7512
14 mm	035.9514S	035.8514S	061.7314	061.7514
16 mm	035.9516S	035.8516S	061.7316	061.7516
18 mm	035.9518S	035.8518S	061.7318	061.7518

Implant Drivers



Medium, L 26 mm
066.4207

VeloDrill™
Alignment Pins
Depth Gauges
Profile Drills

Drill No. 6

	Ø 4.2 mm	
	Short, L 34 mm	066.1306
	Medium, L 38 mm	066.1506
	Long, L 42 mm	066.1706
	Depth Gauge	046.804
	Profile Drills, Ø 4.5 mm	034.365

Drill No. 7

	Ø 4.7 mm	
	Short, L 34 mm	066.1307
	Medium, L 38 mm	066.1507
	Long, L 42 mm	066.1707
	Depth Gauge	046.805
	Profile Drills, Ø 5.0 mm	034.382

WB (Wide Base)

Closure Cap
H 0.4 mm / 2 mm



064.8102S



064.8103S

Healing Abutment



AH = abutment height
GH = gingiva height
Ø = diameter

Healing Abutments for Crown, AH 2 mm

GH	Diameter (Ø) Ø 4.0 mm	Ø 5.0 mm	Ø 6.5 mm	Ø 7.5 mm
				
1.5 mm	064.4202S	064.4212S	064.4222S	–
2.5 mm	064.4204S	064.4214S	064.4224S	064.4234S*
3.5 mm	064.4206S	064.4216S	064.4226S	064.4236S*

Healing Abutments for Crown, AH 4 mm

GH	Diameter (Ø) Ø 4.0 mm	Ø 5.0 mm	Ø 6.5 mm	Ø 7.5 mm
				
1.5 mm	064.4203S	064.4213S	064.4223S	–
2.5 mm	064.4205S	064.4215S	064.4225S	064.4235S*
3.5 mm	064.4207S	064.4217S	064.4227S	064.4237S*

Auxiliary Instruments

Abutment removal kit

RB/WB Abutment-Removal Screw		to push out Abutments, which cannot be removed from the implant due to friction, TAN	065.0007
Removal Tool		for BLX Basal Screw, left-hand, length 27 mm, stainless steel	065.0008
		for BLX Basal Screw, left-hand, length 21 mm, stainless steel	065.0009

Ø 5.5 mm

BLC

WB (Wide Base)



BLX

WB (Wide Base)



Ø 6.5 mm

BLC

WB (Wide Base)



BLX

WB (Wide Base)



	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®	Roxolid® SLActive®	Roxolid® SLA®
6 mm	035.9706S	035.8706S	061.8306	061.8506	035.9806S	035.8806S	061.9306	061.9506
8 mm	035.9708S	035.8708S	061.8308	061.8508	035.9808S	035.8808S	061.9308	061.9508
10 mm	035.9710S	035.8710S	061.8310	061.8510	035.9810S	035.8810S	061.9310	061.9510
12 mm	035.9712S	035.8712S	061.8312	061.8512	035.9812S	035.8812S	061.9312	061.9512
14 mm	035.9714S	035.8714S	061.8314	061.8514	035.9814S	—	061.9314	061.9514
16 mm	035.9716S	—	061.8316	061.8516	035.9816S	—	061.9316	061.9516
18 mm	—	—	—	—	—	—	—	—



Long, L 31 mm
066.4202



Short, L 21 mm
066.4205



Long, L 31 mm
066.4206

Drill No. 8



Ø 5.2 mm	
Short, L 34 mm	066.1308
Medium, L 38 mm	066.1508
Long, L 42 mm	–
Depth Gauge	046.806
Profile Drills, Ø 5.5 mm	034.366

Drill No. 9



Ø 6.2 mm	
Short, L 34 mm	066.1309
Medium, L 38 mm	066.1509
Long, L 42 mm	–
Depth Gauge	046.807
Profile Drills, Ø 6.5 mm	034.367

WB (Wide Base)



064.8102S



064.8103S

Healing Abutments for Crown – Wide Profile, AH 2 mm

	Diameter (⌀)	
GH	Ø 6.0 mm	Ø 7.5 mm
0.75 mm	064.8201S	064.8203S
1.5 mm	064.8212S	064.8214S

Healing Abutments for Crown – Wide Profile, AH 4 mm

	Diameter (⌀)	
GH	Ø 6.0 mm	Ø 7.5 mm
0.75 mm	064.8202S	064.8204S
1.5 mm	064.8213S	064.8215S

Healing Abutment for Bridge, AH 2 mm

	Diameter (⌀)
GH	Ø 5.0 mm
1.5 mm	064.4232S

Healing Abutment for Bridge, AH 4 mm

	Diameter (⌀)
GH	Ø 5.0 mm
1.5 mm	064.4233S

Selection guide for the Straumann® Modular Cassette and instruments

The Straumann® Modular Cassette Selection Guide helps to define the required Modular Cassette parts and instruments needed for a specific indication. Each chapter includes an order list as well as a set-up overview which shows how to assemble the parts. Art. Nr. 707824

BLX/BLC PROSTHETICS

RB/WB prosthetics – fit on all BLX/BLC implants (Ø 3.3 mm – Ø 6.5 mm)

- crowns with slim emergence profiles
- bridges

Impression Posts
Impression Caps
Implant Analogs

Abutment Level

Implant Analog for Screw-retained Abutments, Ø 4.6 mm, 0°



023.4756

Open-tray Impression for Screw-retained Abutments, Ø 4.6 mm



Crown 025.2244
Bridge/Bar 025.0012

Closed-tray Impression for Screw-retained Abutments, Ø 4.6 mm



Crown 025.2246
Bridge/Bar 025.0014

Digital Impression Posts
Scanbodies and Repositionable Analogs

Metal Scanbody for Screw-retained Abutments, Ø 4.6 mm




025.0081

Repositionable Implant Analog for Screw-retained Abutments, Ø 4.6 mm



025.0008

Temporary Abutments




AH = abutment height
GH = gingiva height
Ø = diameter

Temporary Titanium Coping for Screw-retained Abutments, Ø 4.6 mm

		Ø 4.6 mm (RB/WB)
	Crown	024.0023
	Bridge	024.0024
Replacement screw		023.4763

Protective Caps

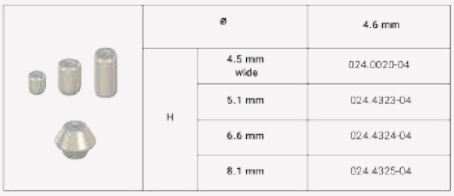

	Ø	4.6 mm
H	4.5 mm wide	024.0020-04
	5.1 mm	024.4323-04
	6.6 mm	024.4324-04
	8.1 mm	024.4325-04

Screw-retained Abutments Variobase® XC



AH = abutment height
GH = gingiva height
Ø = diameter


Screw-retained Abutments

		Ø 4.6 mm (RB/WB)		
	Angle	0°	17°	30°
	GH 0.75 mm	–	–	
	GH 1.5 mm	062.4722S		
	GH 2.5 mm	062.4723S		
	GH 3.5 mm	062.4724S	062.4733S	062.4743S
	GH 4.5 mm	062.4725S	062.4734S	062.4744S
	GH 5.5 mm	–	062.4735S	062.4745S
Replacement screw		065.0036		

RB/WB SRA PLAN Abutment, POM

0°	17°	30°
		
025.0073V4	025.0074V4	025.0075V4

CARES® Abutments
Titanium Abutments
Gold Abutments
Hybrid Abutments



AH = abutment height
GH = gingiva height
Ø = diameter

Burn-out Copings, Plastic

	Ø 4.6 mm
Crown	023.4748
Bridge	023.4758
incl. screw 023.4763	

Titanium Copings

	Ø 4.6 mm
	
Crown	023.4747
Bridge	023.4751
Bar	023.4752
incl. screw 023.4763	

Variobase® for Bridge/Bar Cylindrical

	Ø 4.6 mm
	023.0028
	incl. screw 023.4763
	Burn-out Coping for Variobase® for Bridge/Bar Cylindrical Coping
	023.0032

Occlusal Screw

	023.4763

Variobase® XC

for Crown	for Bridge/Bar	for Bridge/Bar AS
Ø 4,6 mm		
		
023.0038	023.0040	023.0041

Implant Level

Analog



065.0021

Open-tray



065.0031



065.0033

Closed-tray



065.4310

Strauman Metal Scanbody



065.0103

Repositionable Implant Analog



065.0023

ScanPost for CEREC™ workflow



065.0038

Temporary Abutments for Crown, AH 10 mm

			Ø 3.8 mm (RB/WB)	Ø 4.5 mm (RB/WB)	Ø 6.0 mm (RB/WB)
	GH	1.5 mm	064.4362	064.4372	–
		2.5 mm	064.4363	064.4373	064.4382
		3.5 mm	064.4364	064.4374	064.4383
Replacement screw			065.0036		

Temporary Abutments for Bridge, AH 10 mm

			Ø 4.5 mm (RB/WB)
	GH	1.5 mm	064.4352
Replacement screw			065.0036

Variobase® XC for Crown, AH 7 mm

			Ø 3.8 mm (RB/WB)	Ø 4.5 mm (RB/WB)
	GH	1.5 mm	062.5017	062.5020
		2.5 mm	062.5018	062.5021
		3.5 mm	062.5019	062.5022
Replacement screw			065.0036	

Variobase® XC for Bridge/Bar, AH 7 mm

			Ø 3.8 mm (RB/WB)	Ø 4.5 mm (RB/WB)
	GH	1.5 mm	062.5065	062.5068
		2.5 mm	062.5066	062.5069
		3.5 mm	062.5067	062.5070
Replacement screw			065.0036	

Burn-out Coping for Variobase® XC for Crown

	Ø 3.8 mm (RB/WB)	Ø 4.5 mm (RB/WB)
	065.0106	065.0107

Burn-out Coping for Variobase® XC for Bridge/Bar

	Ø 3.8 mm (RB/WB)	Ø 4.5 mm (RB/WB)
	065.0131	065.0132

Anatomic Abutments

			Ø 6.0 mm (RB/WB)	
	Angle		0°	17°
	GH	2.5 mm	062.4103	062.4153
		3.5 mm	062.4104	062.4154
Replacement screw			065.0036	

RB/WB Pre-Milled Abutment Blanks

	Medentika Holder Ø 11.5 mm	Medentika Holder Ø 15.8 mm	CARES Ø 12 mm
	062.4601	062.4602	062.4603

BLX/BLC PROSTHETICS


RB/WB prosthetics – fit on all BLX/BLC implants (Ø 3.3 mm – Ø 6.5 mm)

- crowns with slim emergence profiles
- bridges

Impression Posts
Impression Caps
Implant Analogs

Digital Impression Posts
Scanbodies and
Repositionable Analogs

Temporary Abutments



AH = abutment height
GH = gingiva height
Ø = diameter

Screw-retained Abutments
Variobase® XC



AH = abutment height
GH = gingiva height
Ø = diameter

Variobase® XC for Crown AS, AH 7 mm

			Ø 4.5 mm (RB/WB)
	GH	1.5 mm	062.5009
		2.5 mm	062.5010
		3.5 mm	062.5011
Replacement screw			065.0037

Variobase® XC for Bridge/Bar AS, AH 7 mm

			Ø 4.5 mm (RB/WB)
	GH	1.5 mm	062.5073
		2.5 mm	062.5074
		3.5 mm	062.5075
Replacement screw			065.0037

Variobase® C

		Ø 3.8 mm (RB/WB)	Ø 4.5 mm (RB/WB)
 GH	1.5 mm	062.4981	062.4982
	2.5 mm	062.4928	062.4930
	3.5 mm	062.4929	062.4931
Replacement screw		065.0036	


Burn-out Coping for Variobase® XC for Crown AS

	Ø 4.5 mm (RB/WB)
	065.0112

Burn-out Coping for Variobase® XC for Bridge/Bar AS

	Ø 4.5 mm (RB/WB)
	065.0135

CARES® Abutments
Titanium Abutments
Gold Abutments
Hybrid Abutments



AH = abutment height
GH = gingiva height
Ø = diameter

Novaloc®

			Ø 3.8 mm (RB/WB)	
	Angle		0°	15°
	GH	1.5 mm	062.4501	–
		2.5 mm	062.4502	062.4507
		3.5 mm	062.4503	062.4508
		4.5 mm	062.4504	062.4509
		5.5 mm	062.4505	062.4510
		6.5 mm	062.4506	062.4511
		7.5 mm	–	062.4512
Replacement screw			065.0036	

Processing Package titanium

	2010.601-STM

Processing Package PEEK

	2010.611-STM

WB prosthetics

fit only on WB implants (⌀4.5 mm - ⌀6.5 mm)

- crowns with wide emergence profiles

Implant Level

Analog



065.0022

Open-tray



065.0032



065.0034

Closed-tray



065.4810

Repositionable Implant Analog



065.0024

Temporary Abutments for Crown, AH 11 mm

			⌀ 5.5 mm (WB)
	GH	0.75 mm	064.4391
		1.5 mm	064.4392
Replacement screw			065.0036

Variobase® XC for Crown, AH 7 mm

			⌀ 5.5 mm WB	⌀ 6.5 mm WB
	GH	0.75 mm	062.5023	—
		1.5 mm	062.5024	062.5061
		2.5 mm	062.5059	062.5062
Replacement screw			065.0036	

Variobase® XC for Crown AS, AH 7 mm

			⌀ 5.5 mm WB	⌀ 6.5 mm WB
	GH	0.75 mm	062.5012	—
		1.5 mm	062.5013	062.5063
		2.5 mm	062.5060	062.5064
Replacement screw			065.0037	

Variobase® XC for Bridge/Bar, AH 7 mm

			⌀ 5.5 mm WB
	GH	0.75 mm	062.5071
		1.5 mm	062.5072
Replacement screw			065.0036

Variobase® XC for Bridge/Bar AS, AH 7 mm

			⌀ 5.5 mm WB
	GH	0.75 mm	062.5076
		1.5 mm	062.5077
Replacement screw			065.0037

Variobase® C

			⌀ 5.5 mm WB
	GH	0.75 mm	062.5032
		1.5 mm	062.4983
Replacement screw			065.0036

WB Pre-Milled Abutment Blanks

	Medentika Holder ⌀ 11.5 mm	Medentika Holder ⌀ 15.8 mm	CARES ⌀ 12 mm
	062.4605	062.4606	062.4607

Burn-out Coping for Variobase® XC for Crown

	⌀ 5.5 mm WB	⌀ 6.5 mm WB
	065.0108	065.0124

Burn-out Coping for Variobase® XC for Bridge/Bar

	⌀ 5.5 mm WB
	065.0133

Burn-out Coping for Variobase® XC for Crown AS

	⌀ 5.5 mm WB	⌀ 6.5 mm WB
	065.0113	065.0126

Burn-out Coping for Variobase® XC for Bridge/Bar AS

	⌀ 5.5 mm WB
	065.0136


Первинне закриття імплантатів

Примітка: Оскільки закриваючі гвинти BLX охоплюють все плече імплантату, рекомендується ретельно очистити з'єднання імплантат-гвинт перед встановленням гвинта та перевірити правильність посадки перед закриттям рани, візуально або за допомогою рентгену.

BLX Implant Closure Caps, sterile		
RB Closure Cap	WB Closure Cap	
		
BLX Implant Ø 3.5 BLX Implant Ø 3.75 BLX Implant Ø 4.0 BLX Implant Ø 4.5	BLX Implant Ø 5.0 BLX Implant Ø 5.5 BLX Implant Ø 6.5	Compatibility
hand-tight	hand-tight	Recommended tightening torque
064.4100S	064.8102S	Article number
Titanium	Titanium	Material

Концепція єдиної платформи

- Один ортопедичний ряд.
  Абатменти RB/WB підходять для всіх імплантатів **BLX/BLC**.
- Виключення абатменти WB – тільки для імплантатів з Ø більше 5,0 мм.

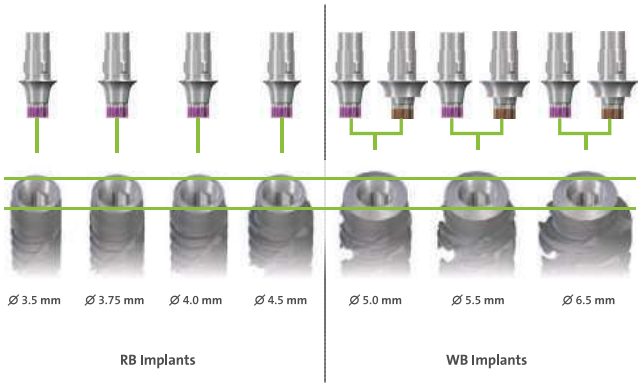

Маркування кольором

Один ортопедичний ряд. Абатменти RB/WB підходять для всіх імплантатів **BLX/BLC**. Виняток абатменти WB – тільки для імплантатів з Ø більше 5,0 мм.

Prosthetic Color		Implant Diameters	Implant Base
	 RB/WB	Ø 3.3 mm Ø 3.5 mm Ø 3.75 mm Ø 4.0 mm Ø 4.5 mm Ø 5.0 mm Ø 5.5 mm Ø 6.5 mm	 RB WB

Prosthetic Color		Implant Diameters	Implant Base
	 WB	**BLX:** Ø 5.0 mm Ø 5.5 mm Ø 6.5 mm **BLC:** Ø 4.5 mm Ø 5.0 mm Ø 5.5 mm Ø 6.5 mm	 WB



Straumann®

TLX/TLC Implant System

Basic Information

Straumann®
TLX/TLC Implant System
System Overview

TLX/TLC SURGERY

Ø 3.3 mm

Standart Plus (SP)

Standart Plus (SP)

Roxolid® SLActive® / SLA®

	TLC NT (Narrow TorcFit)		TLC RT (Regular TorcFit)		TLC NT (Narrow TorcFit)		TLC RT (Regular TorcFit)	
								
	SLActive®	SLA®	SLActive®	SLA®	SLActive®	SLA®	SLActive®	SLA®
6 mm	–	–	–	–	035.7206S	035.6206S	035.7306S	035.6306S
8 mm	035.7008S	035.6008S	035.7108S	035.6108S	035.7208S	035.6208S	035.7308S	035.6308S
10 mm	035.7010S	035.6010S	035.7110S	035.6110S	035.7210S	035.6210S	035.7310S	035.6310S
12 mm	035.7012S	035.6012S	035.7112S	035.6112S	035.7212S	035.6212S	035.7312S	035.6312S
14 mm	035.7014S	035.6014S	035.7114S	035.6114S	035.7214S	035.6214S	035.7314S	035.6314S
16 mm	035.7016S	035.6016S	035.7116S	035.6116S	035.7216S	035.6216S	035.7316S	035.6316S
18 mm	035.7018S	035.6018S	035.7118S	035.6118S	035.7218S	035.6218S	035.7318S	035.6318S

Implant Drivers

Short, L 21 mm		066.4101
Medium, L 26 mm		066.4107
Long, L 31 mm		066.4102
Extra long, L 36 mm		066.4108

VeloDrill Alignment Pins Depth Gauges Profile Drills

Drill No. 1 (Pilot Drill)

	Ø 2.2 mm	
	Short, L 34 mm	066.1301
	Medium, L 38 mm	066.1501
	Long, L 42 mm	066.1701
	Alignment Pin	046.799

Drill No. 2

	Ø 2.8 mm	
	Short, L 34 mm	066.1302
	Medium, L 38 mm	066.1502
	Long, L 42 mm	066.1702
	Alignment Pin	046.800

Profile Drills

NT Ø 3.5 mm	RT Ø 4.8 mm
–	**RT Profile Drill**

	Short 036.3300
	Long 036.3301

Closure Caps

NT Closure Cap

		Ø 2.7 mm	Ø 4 mm
	H 0 mm	036.3200S 036.3200SV4	–
	H 1.5 mm	–	036.0201S 036.0201SVS

RT Closure Cap

		Ø 2.7 mm	Ø 5.5 mm
	H 0 mm	036.3200S 036.3200SV4	–
	H 1.5 mm	–	036.1201S 036.1201SVS

Healing Caps


NT Healing Cap

		Ø 4 mm
	H 2.0 mm	–
	H 3.0 mm	036.0203S
	H 4.5 mm	036.0204S

RT Healing Cap

		Ø 5.5 mm
	H 2.0 mm	036.1202S
	H 3.0 mm	036.1203S
	H 4.5 mm	036.1204S

Auxiliary Instruments

Torque Control Device		066.1100

Ø 3.75 mm

Standart Plus (SP)		Standart (S)	
TLX NT (Narrow TorcFit)		**TLX** NT (Narrow TorcFit)	
			
SLActive®	SLA®	SLActive®	SLA®
035.3006S	035.2006S	035.1006S	035.0006S
035.3008S	035.2008S	035.1008S	035.0008S
035.3010S	035.2010S	035.1010S	035.0010S
035.3012S	035.2012S	035.1012S	035.0012S
035.3014S	035.2014S	035.1014S	035.0014S
035.3016S	035.2016S	035.1016S	035.0016S
035.3018S	035.2018S	035.1018S	035.0018S

Standart Plus (SP)		Standart (S)	
TLX RT (Regular TorcFit)		**TLX** RT (Regular TorcFit)	
			
SLActive®	SLA®	SLActive®	SLA®
035.3106S	035.2106S	035.1106S	035.0106S
035.3108S	035.2108S	035.1108S	035.0108S
035.3110S	035.2110S	035.1110S	035.0110S
035.3112S	035.2112S	035.1112S	035.0112S
035.3114S	035.2114S	035.1114S	035.0114S
035.3116S	035.2116S	035.1116S	035.0116S
035.3118S	035.2118S	035.1118S	035.0118S

Ø 4.5 mm

Standart Plus (SP)			
TLC RT (Regular TorcFit)		**TLC** WT (Wide TorcFit)	
			
SLActive®	SLA®	SLActive®	SLA®
035.7506S	035.6506S	035.7606S	035.6606S
035.7508S	035.6508S	035.7608S	035.6608S
035.7510S	035.6510S	035.7610S	035.6610S
035.7512S	035.6512S	035.7612S	035.6612S
035.7514S	035.6514S	035.7614S	035.6614S
035.7516S	035.6516S	035.7616S	035.6616S
035.7518S	035.6518S	035.7618S	035.6618S

Surgical Handle		066.4000

Drill No. 3

	Ø 3.2 mm	
	Short, L 34 mm	066.1303
	Medium, L 38 mm	066.1503
	Long, L 42 mm	066.1703
	Depth Gauge	046.801
	Profile Drills, Ø 3.3mm	034.362

Drill No. 4

	Ø 3.5 mm	
	Short, L 34 mm	066.1304
	Medium, L 38 mm	066.1504
	Long, L 42 mm	066.1704
	Depth Gauge	046.802
	Profile Drills, Ø 3.75 mm	034.363

NT Ø 3.5 mm

–

NT Closure Cap

		Ø 2.7 mm	Ø 4 mm
	H 0 mm	036.3200S 036.3200SV4	–
	H 1.5 mm	–	036.0201S 036.0201SVS

NT Healing Cap

		Ø 4 mm
	H 2.0 mm	–
	H 3.0 mm	036.0203S
	H 4.5 mm	036.0204S

RT Ø 4.8 mm

RT Profile Drill

	Short 036.3300
	Long 036.3301

RT Closure Cap

		Ø 2.7 mm	Ø 5.5 mm
	H 0 mm	036.3200S 036.3200SV4	–
	H 1.5 mm	–	036.1201S 036.1201SVS

RT Healing Cap

		Ø 5.5 mm
	H 2.0 mm	036.1202S
	H 3.0 mm	036.1203S
	H 4.5 mm	036.1204S

WT Ø 6.5 mm

WT Profile Drill

	Short 036.3302
	Long 036.3303

WT Closure Cap

		Ø 2.7 mm
	H 0 mm	036.3200S 036.3200SV4

WT Healing Cap

		Ø 7.2 mm
	H 2.0 mm	036.2202S
	H 3.0 mm	036.2203S
	H 4.5 mm	036.2204S

Ratchet		046.119

Straumann®
TLX/TLC Implant System
System Overview

TLX/TLC SURGERY

Ø 4.5 mm

	Standart Plus (SP)		Standart (S)		Standart Plus (SP)		Standart (S)	
	TLX NT (Narrow TorcFit)		**TLX** NT (Narrow TorcFit)		**TLX** RT (Regular TorcFit)		**TLX** RT (Regular TorcFit)	
								
	SLActive®	SLA®	SLActive®	SLA®	SLActive®	SLA®	SLActive®	SLA®
Roxolid® SLActive® / SLA ®								
6 mm	035.3406S	035.2406S	035.1406S	035.0406S	035.3506S	035.2506S	035.1506S	035.0506S
8 mm	035.3408S	035.2408S	035.1408S	035.0408S	035.3508S	035.2508S	035.1508S	035.0508S
10 mm	035.3410S	035.2410S	035.1410S	035.0410S	035.3510S	035.2510S	035.1510S	035.0510S
12 mm	035.3412S	035.2412S	035.1412S	035.0412S	035.3512S	035.2512S	035.1512S	035.0512S
14 mm	035.3414S	035.2414S	035.1414S	035.0414S	035.3514S	035.2514S	035.1514S	035.0514S
16 mm	035.3416S	035.2416S	035.1416S	035.0416S	035.3516S	035.2516S	035.1516S	035.0516S
18 mm	035.3418S	035.2418S	035.1418S	035.0418S	035.3518S	035.2518S	035.1518S	035.0518S

Implant Drivers

Short, L 21 mm		066.4201
Medium, L 26 mm		066.4207
Long, L 31 mm		066.4202

VeloDrill
Alignment Pins
Depth Gauges
Profile Drills

Drill No. 5

	Ø 3.7 mm
	Short, L 34 mm — 066.1305
	Medium, L 38 mm — 066.1505
	Long, L 42 mm — 066.1705
	Alignment Pin — 046.803

Drill No. 6

	Ø 4.2 mm	
	Short, L 34 mm	066.1306
	Medium, L 38 mm	066.1506
	Long, L 42 mm	066.1706
	Depth Gauge	046.804
	Profile Drills, Ø 4.5 mm	034.365

Profile Drills

NT Ø 3.5 mm	RT Ø 4.8 mm
–	**RT Profile Drill**  Short 036.3300 / Long 036.3301

Closure Caps

NT Closure Cap

		Ø 2.7 mm	Ø 4 mm
	H 0 mm	036.3200S 036.3200SV4	–
	H 1.5 mm	–	036.0201S 036.0201SVS

RT Closure Cap

		Ø 2.7 mm	Ø 5.5 mm
	H 0 mm	036.3200S 036.3200SV4	–
	H 1.5 mm	–	036.1201S 036.1201SVS

Healing Caps

NT Healing Cap

		Ø 4 mm
	H 2.0 mm	–
	H 3.0 mm	036.0203S
	H 4.5 mm	036.0204S

RT Healing Cap

		Ø 5.5 mm
	H 2.0 mm	036.1202S
	H 3.0 mm	036.1203S
	H 4.5 mm	036.1204S

Auxiliary Instruments

Holding Key		046.064

Ø 5.5 mm

Standart Plus (SP)		Standart Plus (SP)		Standart (S)	
TLC WT (Wide TorcFit)		**TLX** WT (Wide TorcFit)		**TLX** WT (Wide TorcFit)	
					
SLActive®	SLA®	SLActive®	SLA®	SLActive®	SLA®
035.7706S	035.6706S	035.3706S	035.2706S	035.1706S	035.0706S
035.7708S	035.6708S	035.3708S	035.2708S	035.1708S	035.0708S
035.7710S	035.6710S	035.3710S	035.2710S	035.1710S	035.0710S
035.7712S	035.6712S	035.3712S	035.2712S	035.1712S	035.0712S
035.7714S	035.6714S	—	—	—	—
035.7716S	035.6716S	—	—	—	—
—	—	—	—	—	—

Ø 6.5 mm

Standart Plus (SP)		Standart Plus (SP)		Standart (S)	
TLC WT (Wide TorcFit)		**TLX** WT (Wide TorcFit)		**TLX** WT (Wide TorcFit)	
					
SLActive®	SLA®	SLActive®	SLA®	SLActive®	SLA®
035.7806S	035.6806S	035.3806S	035.2806S	035.1806S	035.0806S
035.7808S	035.6808S	035.3808S	035.2808S	035.1808S	035.0808S
035.7810S	035.6810S	035.3810S	035.2810S	035.1810S	035.0810S
035.7812S	035.6812S	035.3812S	035.2812S	035.1812S	035.0812S
035.7814S	035.6814S	—	—	—	—
035.7816S	035.6816S	—	—	—	—
—	—	—	—	—	—

Short, L 21 mm		066.4205

Long, L 31 mm		066.4206

Drill No. 7

	Ø 4.7 mm	
	Short, L 34 mm	066.1307
	Medium, L 38 mm	–
	Long, L 42 mm	066.1707
	Alignment Pin	046.805

Drill No. 8

	Ø 5.2 mm	
	Short, L 34 mm	066.1308
	Medium, L 38 mm	066.1508
	Long, L 42 mm	–
	Depth Gauge	046.806
	Profile Drills, Ø 5.5 mm	034.366

Drill No. 9

	Ø 6.2 mm	
	Short, L 34 mm	066.1309
	Medium, L 38 mm	066.1509
	Long, L 42 mm	–
	Depth Gauge	046.807
	Profile Drills, Ø 6.5 mm	034.367

WT Ø 6.5 mm

WT Profile Drill

	Short 036.3302
	Long 036.3303

WT Closure Cap

		Ø 2.7 mm
	H 0 mm	036.3200S 036.3200SV4

WT Healing Cap

		Ø 7.2 mm
	H 2.0 mm	036.2202S
	H 3.0 mm	036.2203S
	H 4.5 mm	036.2204S

Implant depth gauge		066.2000

Selection guide for the Straumann® Modular Cassette and instruments

The *Straumann® Modular Cassette Selection Guide* (702824/en) helps to define the required Modular Cassette parts and instruments needed for a specific indication. Each chapter includes an order list as well as a set-up overview which shows how to assemble the parts.

Straumann®
TLX/TLC Implant System
System Overview

TLX/TLC PROSTHETICS

NT - Narrow TorcFit™
Ø 3.5 mm



Impression Posts
Digital Impression Posts
Implant Analogs
Scanbodies

Implant Level

Impression Post Open Tray		Impression Post Closed Tray	Implant Analog	Repositionable Implant Analog	Metal Scanbody
					
036.0000	036.0001	036.0002	036.0100	036.1102	036.3230

Temporary Restorations

Temporary Abutment, crown	Temporary Abutment, bridge	Replacement Screw
		
037.0000	037.0001	036.3110

Variobase® XC
Cementable Abutments
Gold Abutments
Burn-out Copings

Variobase® XC for Crown		Variobase® XC for Crown AS		Variobase® XC for Bridge/Bar		Variobase® XC for Bridge/Bar AS		Variobase® C
								
062.5025	065.0109	062.5014	065.0114	062.5003	065.0117	062.4992	065.0120	037.0205

CARES® Abutments
CARES® Screw-retained Bridge

CARES® Abutment*



available in TAN or CoCr

Pre-milled Abutment Blanks

Medentika® Holder 11.5 mm



037.0600

Screw-retained Abutments Copings

Screw-retained Abutment AH 3.5 mm, Ø 4.6 mm, 17°	Screw-retained Abutment AH 3.5 mm, Ø 4.6 mm, 30°	RB/WB Screw-retained PLAN Abutment, 17°	RB/WB Screw-retained PLAN Abutment, 30°	Burn-out Copings, Ø 4.6 mm	
					
037.0410S	037.0411S	025.0074V4	025.0075V4	**Crown** 023.4748	**Bridge** 023.4758

Novaloc®

Novaloc® 0°



H 1 mm	037.0500	H 4 mm	037.0503
H 2 mm	037.0501	H 5 mm	037.0504
H 3 mm	037.0502	H 6 mm	037.0505

Novaloc® Additional Parts

Processing Package, Titanium	Processing Package, PEEK	Matrix Housing, Titanium
		
2010.601-STM	2010.611-STM	2010.701-STM

NT - Narrow TorcFit™
Ø 3.5 mm



Abutment Level

Implant Analog for Screw-retained Abutments, Ø 4.6 mm, 0°



023.4756

Open-tray Impression for Screw-retained Abutments, Ø 4.6 mm



Crown 025.2244
Bridge/Bar 025.0012

Closed-tray Impression for Screw-retained Abutments, Ø 4.6 mm



Crown 025.2246
Bridge/Bar 025.0014

Metal Scanbody for Screw-retained Abutments, Ø 4.6 mm



025.0081

Repositionable Implant Analog for Screw-retained Abutments, Ø 4.6 mm



025.0008

Polishing Aid for Screw-retained Abutments, Ø 4.6 mm



025.0005

Cementable Abutment 0°, for crowns/bridges



037.0100

Crown 037.0110

Bridge 037.0111

Cementable Abutment 15°, for crowns/bridges



037.0101

Crowns/Bridges 037.0112

Replacement Screw

036.3110

Replacement Screw for Variobase® for Crown AS



036.3111

CARES® Screw-retained Bridge*



available in Ti or coron®

Medentika® Holder 15.8 mm



037.0601

CARES® 12 mm



037.0610

Titanium Copings, Ø 4.6 mm



Crown 023.4747



Bridge 023.4751



Bar 023.4752

Variobase® for Bridge/Bar Cylindrical, Ø 4.6 mm



023.0028

023.0032

Variobase® XC

for Crown	for Bridge/Bar	for Bridge/Bar AS
Ø 4,6 mm		
		
023.0038	023.0040	023.0041

Occlusal Screw



023.4763

Lab Processing Screw



L 20mm 025.0006



L 10mm 025.0052

Novaloc® 15°



H 2 mm	037.0510	H 5 mm	037.0513
H 3 mm	037.0511	H 6 mm	037.0514
H 4 mm	037.0512		

Replacement Screw



036.3110

Matrix Housing, PEEK

2010.702-STM

Matrix Housing - Extended



2010.703-STM

Novaloc® Retention Insert

	Red, extra-light	2010.710-STM		Green, strong	2010.713-STM
	White, light	2010.711-STM		Blue, extra-strong	2010.714-STM
	Yellow, medium	2010.712-STM		Black, ultra-strong	2010.715-STM

Straumann®
TLX/TLC Implant System
System Overview

TLX/TLC PROSTHETICS

Straumann® TLX Implant TorcFit™ Connection

RT - Regular TorcFit™
Ø 4.8 mm



Impression Posts
Digital Impression Posts
Implant Analogs
Scanbodies

Impression Post Open Tray



036.1000



036.1001

Impression Post Closed Tray



036.1002

Implant Analog



036.0102

Repositionable Implant Analog



036.2100

Metal Scanbody



036.3230

Temporary Restorations

Temporary Abutment, crown



037.1000

Temporary Abutment, bridge



037.1001

Replacement Screw



036.3110

Variobase® XC
Cementable Abutments
Gold Abutments
Burn-out Copings

Variobase® XC for Crown



062.5026

065.0110

Variobase® XC for Crown AS



062.5015

065.0115

Variobase® XC for Bridge/Bar



062.5004

065.0118

Variobase® XC for Bridge/Bar AS



062.4993

065.0121

Cementable Abutment 0°, for crowns/bridges



037.1100

Crown
037.1110

Bridge
037.1111

Cementable Abutment 15°, for crowns/bridges



037.1101

Crowns/Bridges
037.1112

Variobase® C



037.1205

Replacement Screw



036.3110

Replacement Screw for Variobase® for Crown AS



036.3111

CARES® Abutments
CARES® Screw-retained Bridge

CARES® Abutment*



available in TAN or CoCr

Pre-milled Abutment Blanks

Medentika® Holder 11.5 mm



037.1600

Medentika® Holder 15.8 mm



037.1601

CARES® 12 mm



037.1610

Novaloc®

Novaloc® 0°



H 1 mm	037.1500	H 4 mm	037.1503
H 2 mm	037.1501	H 5 mm	037.1504
H 3 mm	037.1502	H 6 mm	037.1505

Novaloc® 15°



H 2 mm	037.1510	H 5 mm	037.1513
H 3 mm	037.1511	H 6 mm	037.1514
H 4 mm	037.1512		

Replacement Screw



036.3110

Novaloc® Additional Parts

Processing Package, Titanium



2010.601-STM

Processing Package, PEEK



2010.611-STM

Matrix Housing, Titanium



2010.701-STM

WT - Wide TorcFit™
Ø 6.5 mm



Impression Post Open Tray



036.2000



036.2001

Impression Post Closed Tray



036.2002

Implant Analog



036.1100

Repositionable Implant Analog



036.2102

Metal Scanbody



036.3230

Temporary Abutment, crown



037.2000

Temporary Abutment, bridge




037.2001

Replacement Screw




036.3110

Variobase® XC for Crown



062.5027 065.0111

Variobase® XC for Crown AS



062.5016 065.0116

Variobase® XC for Bridge/Bar



062.5005 065.0119

Variobase® XC for Bridge/Bar AS



062.4994 065.0122

Variobase® C



037.2205

Cementable Abutment 0°, for crowns/bridges



037.2100 **Crown** 037.2110 **Bridge** 037.2111

Cementable Abutment 15°, for crowns/bridges



037.2101 **Crowns/Bridges** 037.2112

Replacement Screw

036.3110

Replacement Screw for Variobase® for Crown AS



036.3111

CARES® Screw-retained Bridge*



available in Ti or coron®

* Straumann® CARES® Abtuments can be ordered via the Straumann® CARES® Visual Software or at www.cares.straumann.com, manufactured at the Straumann® CADCAM production center, also available via Straumann® CARES® Scan & Shape Service

Medentika® Holder 11.5 mm



037.2600

Medentika® Holder 15.8 mm



037.2601

CARES® 12 mm



037.2610

Novaloc® 0°



H 1 mm	037.2500	H 4 mm	037.2503
H 2 mm	037.2501	H 5 mm	037.2504
H 3 mm	037.2502	H 6 mm	037.2505

Novaloc® 15°



H 2 mm	037.2510	H 5 mm	037.2513
H 3 mm	037.2511	H 6 mm	037.2514
H 4 mm	037.2512		

Replacement Screw

036.3110

Matrix Housing, PEEK



2010.702-STM

Matrix Housing - Extended




2010.703-STM

Novaloc® Retention Insert

Red, extra-light	2010.710-STM		Green, strong	2010.713-STM	
White, light	2010.711-STM		Blue, extra-strong	2010.714-STM	
Yellow, medium	2010.712-STM		Black, ultra-strong	2010.715-STM	


Імплантат TLX. Конструкція та специфікація

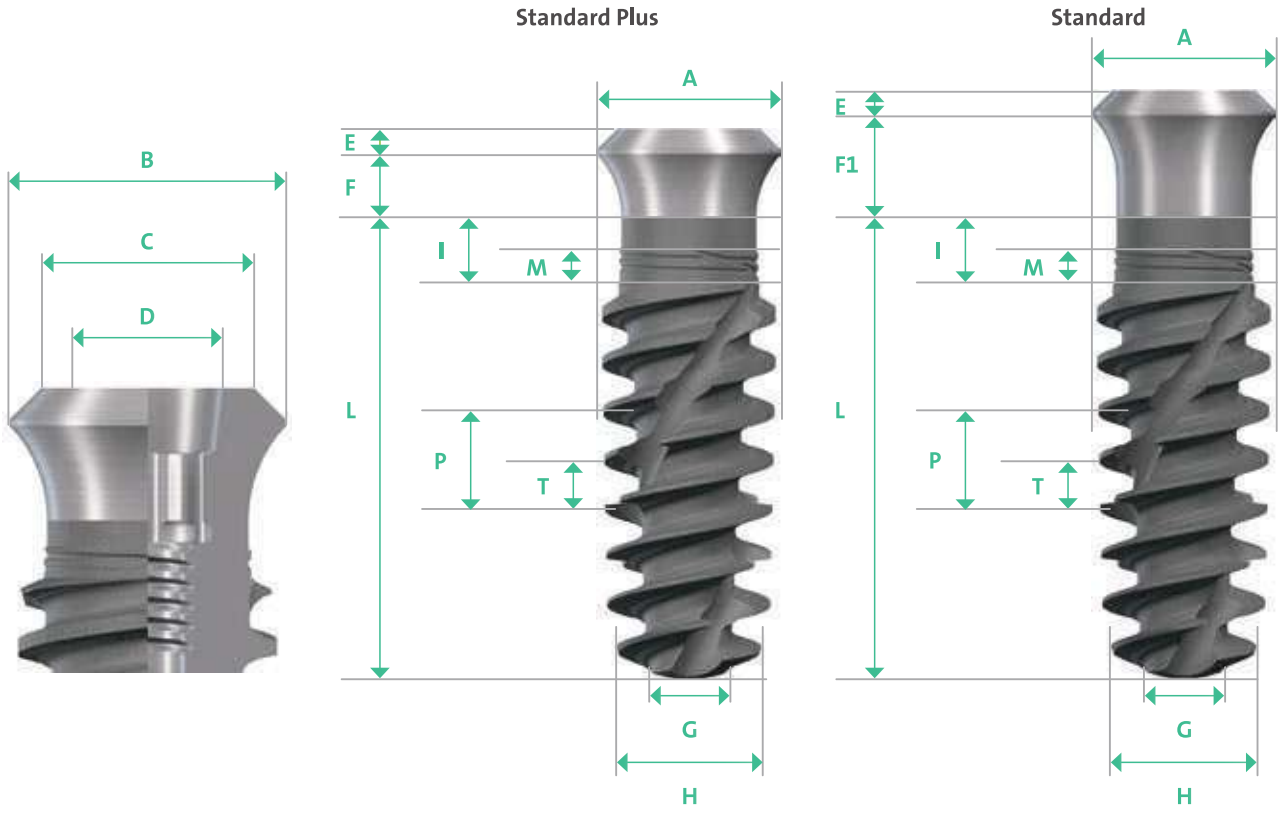

	Straumann® TLX Implant ⌀3.75 mm NT	Straumann® TLX Implant ⌀3.75 mm RT	Straumann® TLX Implant ⌀4.5 mm NT	Straumann® TLX Implant ⌀4.5 mm RT	Straumann® TLX Implant ⌀5.5 mm WT	Straumann® TLX Implant ⌀6.5 mm WT
[A] Maximum outer diameter	⌀3.75 mm		⌀4.5 mm		⌀5.5 mm	⌀6.5 mm
[B] Shoulder diameter	⌀3.5 mm	⌀4.8 mm	⌀3.5 mm	⌀4.8 mm	⌀6.5 mm	
[C] Platform diameter	⌀2.9 mm	⌀3.7 mm	⌀2.9 mm	⌀3.7 mm	⌀5.0 mm	
[D] Connection diameter	⌀2.7 mm					
[E] 45° bevel height	0.5 mm					
[F] Smooth shoulder height* Standard Plus (SP)	1.8 mm					
[F1] Smooth shoulder height* Standard (S)	2.8 mm					
[G] Apical diameter, body	⌀1.9 mm				⌀2.0 mm	⌀3.0 mm
[H] Apical diameter, threads	⌀2.9 mm		⌀3.6 mm		⌀4.0 mm	⌀5.2 mm
Number of apical cutting edges	2			4		
[L] Implant lengths: 6 mm, 8 mm						
[I] Threads to shoulder height	1.0 mm					
[M] Micro threads height	0.5 mm					
[P] Thread pitch**	1.7 mm		2.0 mm		2.1 mm	2.5 mm
[T] Thread spacing	0.85 mm		1.0 mm		1.05 mm	1.25 mm
[L] Implant lengths: 10 mm, 12 mm, 14 mm						
[I] End of threads to shoulder distance	1.7 mm					
[M] Micro threads height	0.85 mm					
[P] Thread pitch**	2.2 mm		2.5 mm			2.8 mm
[T] Thread spacing	1.1 mm		1.25 mm			1.4 mm
[L] Implant lengths: 16 mm, 18 mm						
[I] Threads to shoulder height	2.0 mm				NA	
[M] Micro threads height	1.0 mm					
[P] Thread pitch**	2.6 mm		2.8 mm			
[T] Thread spacing	1.3 mm		1.4 mm			

* This quote refers to height of the shoulder with a smooth non-SLActive® surface
** Implant advances by this distance with every full rotation (360°)

Імплантат TLC. Конструкція та специфікація

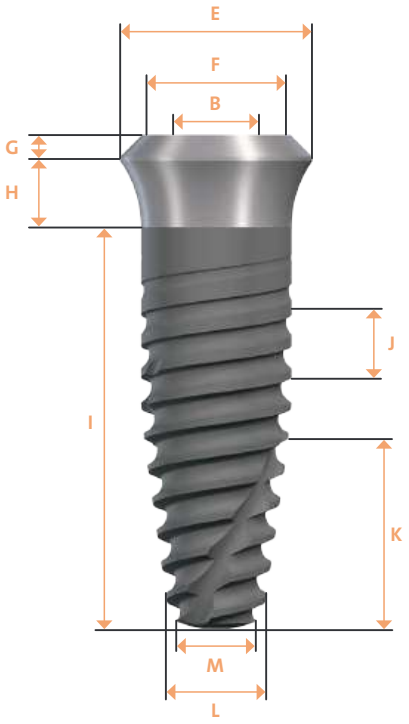


	Straumann BLC™ and TLC™ Implants							
	TLC Ø 3.3 mm NT	TLC Ø 3.3 mm RT	TLC Ø 3.75 mm NT	TLC Ø 3.75 mm RT	TLC Ø 4.5 mm RT	TLC Ø 4.5 mm WT	TLC Ø 5.5 mm WT	TLC Ø 6.5 mm WT
(A) Maximum implant body outer diameter	3.3 mm		3.75 mm		4.5 mm		5.5 mm	6.5 mm
(B) Connection diameter	2.7 mm							
(E) Shoulder diameter	3.5 mm	4.8 mm	3.5 mm	4.8 mm	4.8 mm	6.5 mm	6.5 mm	
(F) Platform diameter	2.9 mm	3.7 mm	2.9 mm	3.7 mm	3.7 mm	5.0 mm	5.0 mm	
(G) 45° bevel height	0.3 mm	0.65 mm	0.3 mm	0.65 mm	0.65 mm	0.85 mm	0.85 mm	0.75 mm
(H) Smooth shoulder height	1.8mm (SP)				1.8mm (SP)		1.8mm (SP)	
(I) Endosteal lengths	8-18mm		6-18mm				6-16mm	
(J) Thread pitch*/flank lead/ depth	1.6mm/20°/0.35mm				1.8mm/20°/0.45mm		2.1mm/ 20°/0.5mm	2.3 mm/ 20°/ 0.75mm
Number of chip flutes	2				2 for L6mm/4 for L8-18mm		4	
Implant lengths: 6 to 8 mm								
(K) Tapered part/taper	2.6 mm/14°				2.7 mm/14°		2.6 mm/14°	
(L) Apical diameter threads	2.22 mm		2.63 mm		3.5 mm		4.63 mm	5.71mm
(M) Apical diameter core	1.52mm		1.81mm		2.36 mm		3.18mm	3.67 mm
Implant lengths: 10 to 18 mm								
(K) Tapered part/taper	5 mm/8°		5.2 mm/8°		5.5 mm/8°			6.5 mm/8°
(L) Apical diameter threads	2.05 mm		2.37 mm		3.10mm		4.14mm	4.87 mm
(M) Apical diameter core	1.35mm		1.61mm		2.10mm		2.21mm	2.76 mm

* Implant advances by this amount with every rotation.

На компоненти імплантаційної системи Straumann TLX/TLC нанесено просте та послідовне лазерне маркування для швидкого і точного підбору допоміжних елементів.
Ця концепція допомагає легко встановити відповідність між компонентами та спрощує комунікацію між сторонами, залученими до лікувального процесу.

- компоненти з маркуванням NT(Narrow, TorcFit) та однією крапкою сумісні лише з імплантатами TLX/TLC з платформою NT.
- компоненти з маркуванням RT(Regular, TorcFit) та двома крапками сумісні лише з імплантатами TLX/TLC з платформою RT.
- компоненти з маркуванням WT(Wide, TorcFit) та трьома крапками сумісні лише з імплантатами TLX/TLC з платформою WT.

	Prosthetic platform	Implant Diameters	Implant platform
NT •	One dot 	**TLC:** Ø3.3 mm Ø3.75 mm **TLX:** Ø3.75 mm Ø4.5 mm	NT 
RT ••	Two dots 	**TLC:** Ø3.3 mm Ø3.75 mm Ø4.5 mm **TLX:** Ø3.75 mm Ø4.5 mm	RT 
WT •••	Three dots 	**TLC:** Ø4.5 mm Ø5.5 mm Ø6.5 mm **TLX:** Ø5.5 mm Ø6.5 mm	WT 

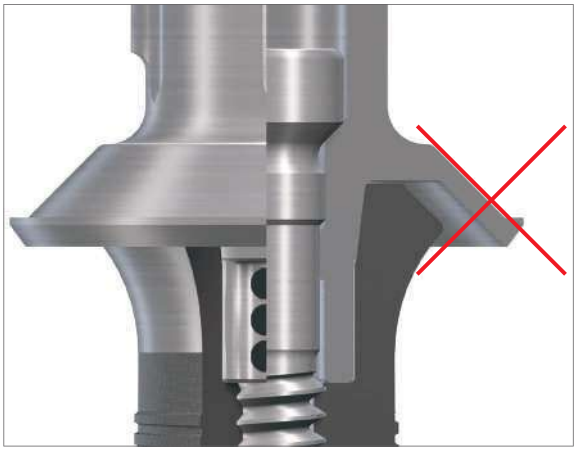

No WT Abutments on NT and RT Implants!
No NT Abutments on RT and WT Implants!
No RT Abutments on NT and WT Implants!

Міжнародна штаб-квартира
Institut Straumann AG
Peter Merian-Weg 12
CH-4002 Базель, Швейцарія
Телефон: +41 (0)61 965 11 11
Факс: +41 (0)61 965 11 01
www.straumann.com

© Institut Straumann AG, 2024. Усі права захищені.
Straumann® та/або інші торгові марки та логотипи Straumann®, згадані в цьому документі,
є товарними знаками або зареєстрованими товарними знаками Straumann Holding AG та/або її дочірніх компаній.